

(19) World Intellectual Property Organization
International Bureau(43) International Publication Date
8 March 2001 (08.03.2001)

PCT

(10) International Publication Number
WO 01/16578 A1(51) International Patent Classification: G01N 21/35,
21/31, A61B 5/00Road, Medfield, MA 02052 (US); CADELL, Theodore,
E. [CA/CA]; 13 Elgin Street East, Conestogo, Ontario N0B
1N0 (CA).

(21) International Application Number: PCT/CA00/01003

(74) Agent: BERESKIN & PARR, 40 King Street West, 40th
Floor, Toronto, Ontario M5H 3Y2 (CA).

(22) International Filing Date: 31 August 2000 (31.08.2000)

(25) Filing Language: English

(81) Designated States (national): CA, JP, US.


(26) Publication Language: English

(84) Designated States (regional): European patent (AT, BE,
CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC,
NL, PT, SE).(30) Priority Data:
60/151,685 31 August 1999 (31.08.1999) US

Published:

(71) Applicant (for all designated States except US): CME
TELEMETRIX INC. [CA/CA]; 560 Parkside Drive,
Waterloo, Ontario N2L 5Z4 (CA).With international search report
Before the expiration of the time limit for amending the
claims and to be republished in the event of receipt of
amendments

(72) Inventors: and

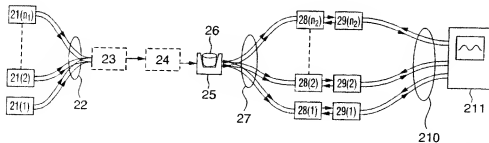(75) Inventors/Applicants (for US only): PAWL/CZYK, Ro-
mund [CA/CA]; 362 Roselawn Place, Waterloo, Ontario
N2L 5P1 (CA); SC/ECINA, Thomas [US/US]; 23 OrndaleFor two-letter codes and other abbreviations, refer to the "Guid-
ance Notes on Codes and Abbreviations" appearing at the begin-
ning of each regular issue of the PCT Gazette.(54) Title: METHOD FOR DETERMINATION OF ANALYTES USING NEAR INFRARED, ADJACENT VISIBLE SPECTRUM
AND AN ARRAY OF LONGER NEAR INFRARED WAVELENGTHS

(57) Abstract: Described is a method which uses spectral data simultaneously collected in a continuous array of discrete wavelength points of the visible spectrum adjacent to the infrared and near infrared part of the light spectrum. The spectral data is collected using a number of detectors with different sensitivity ranges. Some detectors may be sensitive to visible and, possibly, to part of the near infrared portion of radiation. Spectral data from the infrared spectrum is collected with the infrared detectors, and are in some embodiments insensitive to the visible light.

- 1 -

Title: METHOD FOR DETERMINATION OF ANALYTES USING
NEAR INFRARED, ADJACENT VISIBLE SPECTRUM AND AN
ARRAY OF LONGER NEAR INFRARED WAVELENGTHS

5 FIELD OF INVENTION

 This invention relates to a device and method for determining
and monitoring concentration levels of one or more constituents
within a varying in time, complex multi component structure, (for
example blood constituents in blood sample, tissue or body parts) or,
10 in particular, blood and tissue constituents in living subjects such as
humans or animals.

BACKGROUND OF INVENTION

 The application of spectroscopy for chemical analysis is well
known. For many years, however, it was mainly used for atomic
15 analysis because sufficiently sensitive detectors did not exist for
infrared, where information on vibration states of the molecules
(especially those of organic origin) is located. Advances in technology
of IR detectors have dramatically changed the situation and presently a
large number of detectors, instruments and methods exist for such
20 applications. This has also opened the way for new applications, but
has imposed new requirements on the technology. One of the most
important applications is a noninvasive analysis of chemical
compositions of living subjects.

 It is generally appreciated that light in spectral range 500nm to
25 770nm belongs to the visible part of the spectrum but, since it does not
cover whole visible range and it is directly adjacent to the infrared part
of the spectrum, herein it is referred to as adjacent visible (AV). It is
widely accepted that of the infrared part of the electromagnetic
spectrum (IR) is divided into the near infrared (NIR), which expands
30 beyond the visible to about 2700 nm, the middle infrared radiation
(MIR), which expands beyond the NIR range and a further expanding
far infrared range (FIR). There are some photodetectors (mainly
silicon) whose sensitivity covers the visible part of spectrum and initial
part of NIR. Therefore, part of visible range adjacent to NIR and part

- 2 -

of NIR adjacent to visible will be referred here as AV/NIR, while the remaining part of NIR range will be referred to as the "longer wavelength NIR region" or "LWNIR".

Non-Invasive Techniques

5 Previous devices for non-invasively monitoring concentration of blood constituents of a patient are known. Usually, a sensor is used to externally measure either the concentration of the constituents in gases emitted by the body or contained in the perspiration, or the concentration of the constituents contained in body fluids such as tears, saliva, or urine. Alternatively, the blood constituents are identified by measurement of attenuation of some radiation passed through a part of a patient's body such as an earlobe, a finger or skin. In majority cases, radiation is measured at one, two or limited number of relatively narrow spectral bands obtained from separate, narrow band light sources (see for example US 4,655,225; US 4,883,953; and US 4,882,492). Some of these devices perform measurements at limited number relatively narrow spectral bands consecutively selected from spectrally broad light by a set of exchangeable narrow-band spectral filters. Analysis of absolute and relative changes in light intensity at these bands under certain conditions may provide important information on body constituents. Exchange of the filters and time required for their stabilization to obtain precise measurement, very often significantly increase duration of the measurement process and as a result, the measurement in different bands are taken with significant time delays. Because of physiological variability of physical state of the alive person, this leads to situation when measurements at different wavelengths are taken under changed physical conditions of the body, making impossible to measure the constituents of the body. Another source of the error in the systems with limited number of discrete spectral bands is wavelength shift of the selected bands from measurement to the measurement and from instrument to the instrument. There are some medical and other applications when these two sources of the error make measurement of constituents impossible. In such a case it

- 3 -

becomes important to make the measurement in whole spectrum virtually simultaneously and to preserve as complete as possible information on whole spectrum. This is achieved applying other techniques, which measure either a full spectrum of light interacting with sample, with a large number (for example, 128 or 256) of wavelengths in a specific range and those that measure a limited number of wavelengths. Those that measure full spectra typically use the wavelengths in the AV/NIR range (see for examples US 5,361,758 and US 4,975,581), where arrays of the photodetectors, produced with application of well established silicon technology, have been available for long time for simultaneous registration of the spectra in large number of discrete points. There are several advantages in measurement of whole spectrum. One of them consists in that the spectra provide information about the desired analyte as well as information about interfering substances (e.g., other analytes) and effects (e.g., light scattering). The second advantage is capability to register a complete information on spectrum even if it is shifted due to temperature changes of sample. Finally, the third advantage is that even if the instrument loses wavelength calibration, whole information is still preserved in the spectrum and can be easily extracted once new wavelength calibration data is available. In some cases, however, there is not enough information available in the above range or available information is insufficient for precise measurement of body constituents and additional information outside the above mentioned spectral range (usually at longer wavelengths) is required.

In some cases, the methods that take measurements at limited number of wavelengths only within the 1100 to 1700nm region can be sufficient, because of the sharper analyte spectra that exist in this region. In majority cases, however, while they provide information relating to the analyte of interest, there is not enough independent information on other analytes whose absorption spectra interferes with that of the desired analyte. In some cases additional information obtained in earlier mentioned spectral range 580nm to 1100nm helps to

- 4 -

eliminate ambiguity introduced by interfering analytes. It is clear that if the sample demonstrates a temporal variability, a simultaneous measurement in whole spectral range of the interest is preferred, to eliminate possible errors caused by changes in the sample.

5 Furthermore, as in earlier discussed cases for shorter spectral range, spectral measurement in limited number of points within 1100nm to 1700nm spectral range in some cases may not be sufficient for recognition of desired analyte. In addition, the measurements usually are very sensitive to both: variations of spectral position of the
10 selected points and width and shape of spectral bands measured at those points. Thus, the methods when measurement in different parts of spectrum are taken at different time, or from different part of samples or within limited number of points may not be sufficient for precise analysis of constituents of the samples and more advanced
15 instruments are required. The way to eliminate these limitations and provide instrument suitable for such measurements is given in this invention. Overall, previous non-invasive devices and techniques have not been sufficiently accurate to be used in place of invasive techniques in the measurement of blood constituent concentration in
20 patients. Some of them have been designed to measure one component only and physical changes to the instrument have to be applied to adapt them to measurement of different components. For some devices it takes unreasonably long time to produce a results; or, some other cannot produce results in an easy-to-use form; or, they
25 cannot measure concentration of two or more constituents simultaneously. Obviously, if the device gives an inaccurate reading, disastrous results could occur for the patient using the device to calculate, for example, dosages for insulin administration.

30 It has been recognized that simultaneous spectrum collection is possible only by applying a large number of photodetectors. Technically this is brought about by spatial dispersion of radiation, composed of different wavelengths, by means of a dispersing device (diffraction grating, for example) and registration of its intensity with

- 5 -

an array of photodetectors. In such cases, the signal registered by each detector of the array can be read virtually simultaneously. This technique has been recognized and many spectrometers with an array of photodetectors are available on the market. Unfortunately, the available arrays systems have various limitations, therefore, the capabilities of such spectrometers are limited.

The most important limitation for each array is its sensitivity range, which is determined by the material used to produce an array. The sensitivity range determines in what spectral range the instrument built with an application of a particular array can work. Grating spectrometers designed with the application of arrays of photodetectors have further intrinsic limitations, which put even stronger constraints on the performance of the instruments. One such constraint is the existence of additional diffraction orders in light diffracted by a grating. The existence of the second order imposes the condition that the spectral range of an array-based instrument cannot be wider than one octave, unless a special filter is placed in front of the array. Production of such filters is not easy, hence, instruments are built to cover less than one octave and a cut-off filter, eliminating radiation with shorter wavelengths is normally used to eliminate the impact of that order. As a result, the spectral range of existing array-based instruments is such that the longest measured wavelength of analyzed light is always smaller than the doubled length of the shortest wavelength analyzed by the spectrometer

Finally, since the number of elements in an array and length of an array are limited, very often it is impossible to achieve high resolution even in that limited spectral range. As a result, the performance of array-based instruments is a compromise between such factors and consequently spectrometers very often cannot provide information needed for particular applications. If, in addition, these applications require simultaneous registration of the wider spectrum (as, for example, non-invasive in-vivo diagnostic), the measurement problem remains unsolved.

- 6 -

SUMMARY OF THE INVENTION

While for some applications relatively simple instruments, measuring of infrared radiation at one or small number of wavelengths are sufficient, it was discovered that for more demanding applications, such as, for example, glucose concentration in blood in a human body, significantly more advanced instruments are required. In particular it has been found that for such applications it is important to collect data in a wide spectral range covering at least part of near infrared and adjacent to it visible part of the spectrum. It has been also discovered that for living subject it is crucial that information is collected simultaneously in whole spectral range of the interest, otherwise physiological changes in the organism during measurement may significantly contribute to the measurement error. Finally, it has been found that because of dependence of the molecular vibration spectrum on temperature it is important to have as complete information on the spectrum as possible. Therefore a need has arisen to build a spectroscopic system able to simultaneously collect information in as wide spectrum as possible. This approach excludes techniques when a spectrum of light is collected with the application of any scanning instrument like those with rotated gratings or Fourier transform spectrometers.

Accordingly, the present invention provides a method for monitoring the concentration level of a particular constituent in a sample or, alternatively, of measuring the concentration level of one or more different constituents using a non-invasive device with higher precision and in a short period of time, through simultaneous measurement of light signal in several different spectral ranges using separate array-based spectrometers.

The present inventors have determined that analyte measurement accuracy with spectral devices measuring full spectra absorption/reflectance in the AV/NIR region, is enhanced by adding to such measurement, measurements from one or more arrays of wavelength in the infrared region

- 7 -

In its broad aspect the present invention provides a method for monitoring the concentration level of a constituent in sample comprising placing the sample in a non-invasive device capable of emitting radiation; directing the radiation onto the sample; measuring radiation collected from the sample; calculating the concentration level based on the measured radiation wherein the radiation directed onto the tissue and collected from the tissue is of the wavelengths starting at 500nm and expanding into AV/NIR range, and wavelengths in the LIR range possible from 1100 to 1700nm.

According to one embodiment, the present invention provides a method for measuring concentration levels of blood constituents within a living subject such as humans or animals, wherein, a polychromatic light source or other single or multiplicity of radiation sources are used that emit a broad spectrum of light in the required range. A number of spectrum analyzing systems containing photodetector arrays, possible sensitive in different spectral ranges provide sensitivity and resolution over portions of the range of the interest, preferably one from 500-1100nm and one from 900-1700nm and further spectral ranges. The method comprises the steps of:

- directing light at a continuum wavelengths (whether from one or more sources) simultaneously onto a sample or a part of a subject;
- collecting the continuum of light after the light has been directed onto and interacted with the sample or the part;
- dividing of collected light into at least two parts separately directed to the corresponding number of spectrum analyzing systems, at least one for AV/NIR and at least another one for WNIR,
- forming of each part of light into a light beam, suitable for simultaneous analysis of corresponding spectral content of each part, preferably by means of a dispersing element, preferable diffraction grating,
- spatially dispersing a portion of the continuum of light predestined for analysis with separate spectrum analyzing systems into a dispersed spectrum of component wavelengths in each selected part,

- 8 -

- forming of dispersed light in each part into light beam suitable for detection with a suitable array of photodetectors,
- the arrays of the photodetectors taking measurement of dispersed light in selected part or whole AV/NIR spectral range and at least one or more arrays applied for measurements of at least selected part or whole LWNIR spectral range.

Preferably these measurements are taken simultaneously or sequentially, or in any combination thereof. The measurement results are transferred to a microprocessor, and the concentration level of said at least one constituent of the sample, in particular of said blood or tissue is calculated and a result of each concentration level is produced.

According to another embodiment of the invention, there is provided a non-invasive device measuring concentration levels of constituents occurring in the sample in particular in blood and tissue in a subject such as a human or animal uses one or more radiation sources. The broad spectrum of light in the adjacent visible spectrum and near infrared range provided by the radiation or light source(s) is/are powered by one or a required number of stabilized power sources. The device (or devices) has a receptor shaped so that a sample or a part of the subject can be placed in contact with the receptor. The receptor has means for eliminating extraneous light and is located relative to the light source (or sources) so that when a sample or body part (or tissue) is placed in contact with the receptor, the source(s) can be activated and light with continuum of wavelengths, is directed onto the part. The device is equipped with means for collecting light in the AV/NIR and LWNIR spectral regions after the light has been directed onto the sample or the part. There are also means for dispersing the collected light over said broad spectrum into a dispersed spectrum of component wavelengths and means for taking measurements of a light signal at many different wavelengths in the AV/NIR and LWNIR regions simultaneously or sequentially. There are also means for transforming results of these measurements over the dispersed spectrum into the concentration of at least one

- 9 -

constituent by using a calibration equation for the at least one constituent. There are also means for determining the concentration level of the at least one constituent of said blood or tissue and then producing a result for each concentration level determined.

5 According to one embodiment of the present invention there is provided a method for determining a concentration of a constituent in a sample comprising the steps of:

 irradiating the sample with a continuum of wavelengths from the adjacent visible and near infrared (AV/NIR) region;

10 collecting radiation after the radiation has been directed onto the part;

 dispersing the continuum of collected radiation into a dispersed spectrum of component wavelengths onto a detector, the detector taking measurements of at least one of transmitted or reflected radiation from the collected radiation; and transferring the measurements to a processor;

15 irradiating the sample with a continuum of wavelengths in the longer wavelength near infrared (LWNIR) region; detecting one or more bands of radiation after the radiation has been directed onto the sample with a detector, the detector taking measurements of at least one of transmitted or reflected radiation ; and

20 transferring the measurements to a processor;
 based on the measurements and one or more calibration algorithms, the processor calculating the concentration of said constituent in said sample, preferably one or more separate energy sources are used to provide radiation.

25 According to another embodiment of the method of the invention the detector of the AV/NIR is one or more spectral instruments with an array of silicon detectors and the detector of LWNIR is one or more spectral instruments with a separate array of infrared sensitive detectors for each band of radiation.

30 According to yet another embodiment the detector of the AV/NIR is one or more spectral instruments with an array of silicon

- 10 -

detectors and the detector of LWNIR is one or more spectral instruments with an array of infrared sensitive detectors and measurements for each band of radiation are taken from appropriate members of the array of infrared sensitive detectors, preferably the
5 infrared sensitive detectors are InGaAs detectors.

According to another embodiment the spectrometers with silicon detectors arrays register light in the all of the visible, visible/infrared and adjacent to visible infrared ranges within the spectral sensitivity range of the detectors, and preferably the
10 spectrometers with infrared sensitive detectors register light in the separate infrared ranges within their spectral sensitivity range.

According to another embodiment of the method all detectors register light in their respectable sensitivity ranges virtually simultaneously.

15 In another aspect of the present invention there is provided a method for determining a concentration of a constituent in a sample comprising the steps of:

irradiating the sample with a continuum of wavelengths from the AV/NIR region;

20 collecting radiation after the radiation has been directed onto the part;

dispersing the continuum of collected radiation into a dispersed spectrum of component wavelengths onto a detector, the detector taking measurements of at least one of transmitted or reflected
25 radiation from the collected radiation; and transferring the measurements to a processor;

irradiating the sample with one or more bands of wavelengths in the LWNIR region; detecting the one or more bands of radiation after the radiation has been directed onto the sample with a detector,
30 the detector taking measurements of at least one of transmitted or reflected radiation ; and

transferring the measurements to a processor;

- 11 -

based on the measurements and one or more calibration algorithms, the processor calculating the concentration of said constituent in said sample, preferably one or more separate energy sources are used to provide radiation.

5 According to another embodiment of the method of the invention the detector of the AV/NIR is one or more spectral instruments with an array of silicon detectors and the detector of LWNIR is one or more spectral instruments with a separate array of infrared sensitive detectors for each band of radiation.

10 According to yet another embodiment the detector of the AV/NIR is one or more spectral instruments with an array of silicon detectors and the detector of LWNIR is one or more spectral instruments with an array of infrared sensitive detectors and measurements for each band of radiation are taken from appropriate members of the array of infrared sensitive detectors, preferably the
15 infrared sensitive detectors are InGaAs detectors.

According to another embodiment the spectrometers with silicon detectors arrays register light in the all of the visible, visible/infrared and adjacent to visible infrared ranges within the
20 spectral sensitivity range of the detectors, and preferably the spectrometers with infrared sensitive detectors register light in the separate infrared ranges within their spectral sensitivity range.

According to another embodiment of the method all detectors register light in their respectable sensitivity ranges virtually
25 simultaneously.

In yet another aspect of the present invention there is provided a method for determining a concentration of a constituent in a sample comprising the steps of:

30 irradiating the sample with a continuum of wavelengths from the AV/NIR region;

collecting radiation after the radiation has been directed onto the part;

- 12 -

dispersing the continuum of collected radiation into a dispersed spectrum of component wavelengths onto a detector, the detector taking measurements of at least one of transmitted or reflected radiation from the collected radiation; and transferring the measurements to a processor;

irradiating the sample with a continuum of wavelengths from the LWNIR region; collecting radiation after the radiation has been directed onto the part;

dispersing the continuum of collected radiation into a dispersed spectrum of bands of radiation onto a detector, the detector taking measurements of at least one of transmitted or reflected radiation; and transferring the measurements to a processor;

based on the measurements and one or more calibration algorithms, the processor calculating the concentration of said constituent in said sample, preferably one or more separate energy sources are used to provide radiation.

According to another embodiment of the method of the invention the detector of the AV/NIR is one or more spectral instruments with an array of silicon detectors and the detector of LWNIR is one or more spectral instruments with a separate array of infrared sensitive detectors for each band of radiation.

According to yet another embodiment the detector of the AV/NIR is one or more spectral instruments with an array of silicon detectors and the detector of LWNIR is one or more spectral instruments with an array of infrared sensitive detectors and measurements for each band of radiation are taken from appropriate members of the array of infrared sensitive detectors, preferably the infrared sensitive detectors are InGaAs detectors.

According to another embodiment the spectrometers with silicon detectors arrays register light in the all of the visible, visible/infrared and adjacent to visible infrared ranges within the spectral sensitivity range of the detectors, and preferably the

- 13 -

spectrometers with infrared sensitive detectors register light in the separate infrared ranges within their spectral sensitivity range.

According to another embodiment of the method all detectors register light in their respectable sensitivity ranges virtually simultaneously.

In accordance with a preferred embodiment of any of the foregoing methods the sample is a finger of a subject.

Other features and advantages of the present invention will become apparent from the following detailed description. It should be understood, however, that the detailed description and the specific examples, while indicating preferred embodiments of the invention, are given by way of illustration only, since various changes and modifications within the spirit and scope of the invention will become apparent to those skilled in the art from this detailed description.

BRIEF DESCRIPTION OF THE DRAWINGS

The invention will now be described in relation to the drawing in which:

Figure 1 shows absorbance spectra from 500-1380 nm for globulins, glucose, urea, creatine, cholesterol and human serum albumin with water displacement compensation.

Figure 2 presents a general concept for simultaneous collection of spectra in a wide spectral range by many array-based instruments, each of which covers a separate spectral range.

DETAILED DESCRIPTION OF THE INVENTION

As used herein "concentration" or "concentration level" means the amount or quantity of a constituent in a solution whether the solution is in vitro or in vivo.

As used herein, "constituent" means a substance, or analyte found in a tissue and includes carbohydrates such as for example glucose, bilirubin, a protein, for examples albumin or , hemoglobin.

As used herein, "in a solution" means in a liquid environment such as, for examples interstitial, or other bodily fluid

- 14 -

As used herein, "tissue" means any tissue of the body of a subject including for example, blood, extracellular spaces, and can mean the entire composition of a body part such as a finger or ear lobe.

As used herein "subject" means any member of the animal kingdom including, preferably, humans.

As noted previously, light in spectral range 500nm to 770nm is referred to herein as adjacent visible (AV). As used herein, the infrared part of the electromagnetic spectrum (IR) is divided into the near infrared (NIR), which expands beyond the visible to about 2700 nm, the middle infrared radiation (MIR), which expands beyond the NIR range and a further expanding far infrared range (FIR). Also, part of visible range adjacent to NIR and part of NIR adjacent to visible will be referred here as AV/NIR, while the remaining part of NIR range will be referred to as the "longer wavelength NIR region" or "LWNIR".

According to a preferred embodiment, in each case, it is assumed that measurement of the light intensity at any given spectral band with given central wavelengths is at a sufficiently high signal to noise ratio in order to achieve the desired results.

As discussed above, the present inventors have determined that significant improvement of the ability to measure analytes in various samples (in tissue in particular) using a non-invasive spectral device can be achieved by adding; it is only necessary to add one or more arrays of wavelength measurements in the LWNIR or IR region to a full spectra absorption measurement in the 500 to 1100nm region to gain a significant improvement in analyte measurement accuracy. In particular analyte measurement accuracy achieved through previous methods is enhanced by adding a full spectra absorption measurement in the 1100 to 1300nm (the "First region") and/or by adding a full spectra absorption measurement in the 1590 to 1700nm (the "Second region") region to a full spectra absorption measurement in the 500 to 1100nm region, preferably in the AV/NIR region, more preferably the addition of the First region to the Second region is performed. The result provides a significant improvement in analyte measurement

- 15 -

accuracy. It will be readily appreciated that the method includes addition of measurements of full spectra absorption from other regions or whole range in the LWNIR or IR.

5 The AV/NIR range has been used because, among other reasons, silicon detectors are sensitive in that range. Silicon detectors, particularly silicon-based detector arrays provide superior noise and dynamic range performance, are readily available, and, are relatively inexpensive. However, the 900 to 1700nm and further IR wavelength ranges provide sharper spectra for many of the analytes of interest as
10 may be seen by referring to Figure 1. An Indium Gallium Arsenite (InGaAs) detector may be used to measure spectra in this region while other detectors array can cover further IR ranges. Unfortunately, these detectors provide inferior noise and dynamic range performance in comparison with silicon, consequently the lower signal to noise ratio
15 offsets some of the advantage of the sharper spectra.

To achieve the advantages of measuring spectra in the IR, one or more arrays of spectra are added to measurements in the AV/ NIR region. The results are significantly better than those achieve with measurements of spectra in either range separately.

20 The light is delivered to the sample or to the tissue, such as a finger, by a suitable conduit such as fiber optics bundle. The light emerging from the finger is collected and delivered to separate sets of detectors by another conduit such as another fiber optics bundle. As just mentioned, a silicon diode array is used to detect light in the
25 AV/NIR region and an InGaAs photodiode array can be used to detect light in the LWNIR region and other detector arrays in further IR ranges. As used herein, "light", "illumination", "radiation" all refer to the light energy provided by a source which is capable of delivering sufficient radiation of a desired wavelength.

30 Any device which is capable of delivering radiation in the ranges of the invention may be utilized and are within the scope of the present invention.

- 16 -

As just mentioned the light source can emit light over a very wide band-width including light in adjacent to infrared visible and the near infrared spectrum. According to one embodiment, the light from the light source (or sources) is delivered by any optical means to the sample, which preferably is placed in an appropriate receptor. In particular the light may pass first through a collimator (a collection of lenses that concentrate the light into a narrow parallel beam directed at the receptor). In another embodiment, when a light scattered sample is tested, the light, in the form of a wide divergent light beam, is delivered by a fiber-optics means directly to a sample or to a receptor containing the sample. An appropriate receptor is shaped to receive a measured sample. Such samples may be, for example, a part of subject being measured, for example, a finger or arm of a human. An appropriate receptor may also be a sample holder in a form of any transparent container or, for some applications, in a form of calibrated cuvette with parallel walls. Alternatively, a receptor could be shaped so that the part of the human or animal, onto which the light is to be directed, is placed near the receptor rather than within the receptor. Further, an integrating cavity may play the role of sample receptor with light coupled into the cavity either directly or by any optical means including optical fibers. After interaction of the light with the sample, the light is collected by any optical means. The light from the sample can be light that has passed through the sample (body part or tissue, for example) or has reflected off it, or a combination thereof. Preferably, the collected light is light that has passed through the sample.

The collected light is divided into a required number of light beams and each of them is directed to a separate spectral analyzing system, preferably an array-based spectrophotometer. Before entering a spectrometer, each light beam may be optionally shaped to a narrow light source by means of suitably distributed fibers or a set of optical elements and a slit. The light from a narrow light source can be either collimated or directly delivered to a diffraction means.

- 17 -

Radiation from a sample interacts with a dispersion means, such as a grating, which disperses the radiation into its component wavelengths so that the light in the AV/NIR region falls along detectors, preferably a length of linear array of silicon of detectors such that light from the LWNIR and other IR regions falls onto the array of detectors, preferably InGaAs detectors. As is readily understood by those skilled in the art, these arrays are comprised of individual detectors and are sensitive in a range of wavelengths which correspond to the AV and IR regions. Preferably, although not necessarily, all detectors are electronically simultaneously scanned to measure signal registered by each individual unit.

The results from the detector are directed to a microprocessor for analysis of the measurements from the detectors and ultimately produces a concentration result for each constituent by applying one of many known chemometric methods such as for example PLS or PCR. The results can be shown on a display and/or printed on a printer. A keyboard allows a user to control the device, for example, to specify a particular constituent to be measured. The timing and control may be activated by the microprocessor to control the device, for example, to determine number and timing of measurements.

The light source or sources can be a quartz-halogen or a tungsten-halogen bulb, supported by any other light source such as a laser or light emitting diodes (LED) (or other light sources able to emit radiation in the required ranges of AV and IR). Any such source is (or are) powered by a stabilized power source, for example, a DC power supply, or by a battery. Preferably, each linear array detector has a sufficient number of photosensitive elements to cover a required spectral range to provide adequate spectral resolution.

A standard measurement procedure comprises taking reference measurements of incident light (being the light generated in the device when no part of the subject is in contact with the receptor) and taking measurements while the sample is present in the receptor. The negative logarithm of the ratio of sample measurement to reference

- 18 -

measurements is then calculated and compared to reference measurements.

Although it should not be construed as a limitation on the method of the invention, the second derivative of measurements may be taken in order to reduce any variation in the result that will be caused by a change in path length for the light.

The noise level within the device may be reduced by a multiple scanning technique whereby the detectors take a number of measurements and then average the results. Preferably, the linear array detector and IR detectors are scanned many times for several repetitions and then the results averaged.

While measuring glucose concentrations is a preferred embodiment of the present invention, the device and method can be used to measure concentration levels of various other constituents found within the blood of humans and animals, for example, amino acids, nitrogen, blood oxygenation, carbon dioxide, cortisol, creatine, creatinine, glucose, ketones, lipids, fat, urea, amino acids, fatty acids, glycosylated hemoglobin, cholesterol, alcohol, lactate, Ca^{++} , K^{+} , Cl^{-} , HCO_3^{-} and HPO_4^{-} , to name a few. Indeed, as will be apparent to those skilled in the art, the method and device can be modified to measure several constituents simultaneously, finally it can be also modified to measure chemical composition of any other materials or samples whose properties may vary in time, demonstrating specific spectral features in AV and IR ranges..

The following is a non-limiting exemplary embodiment of the present invention.

EXEMPLARY EMBODIMENT OF INVENTION

Referring now to Figure 2, a certain number (n_1) of light sources generate a broad spectrum of light covering all required spectral ranges. The light sources contain power supplies, light sources, means to collect light from these sources and means to concentrate light into optical elements predestined to mix light from these sources and bring it to the sample.

- 19 -

Light from the light source is collected by light collecting means, preferably by multiple fiber bundles 22, and is optionally delivered through a light mixing device 23 (glass rod, for example) and, optionally a light forming device 24 (light collimator, or focusing lens, for example) to a sample receptor 25 (sample holder, finger holder, integrating cavity or any other device to hold sample) containing a sample 26 (human finger, for example). After interaction with sample the light is collected by a light collecting device 27 (another light bundle, or any other light collecting optical system, lens, for example) and is divided into as many parts as required to cover all possible spectral bands. Division can be performed either by simple splitting of fibers into multiplicity of fiber optics legs or using wide-band or dichroic beam splitters.

Each "part" of light is directed to separate spectrum analyzing devices 28, preferably array-based spectrometers. The number (n_2) of spectrometers (generally different from the number of light sources) is selected to cover an entire spectral range of interest for a tested sample with demanded resolution.

The light delivering means together with the spectrum analyzing device may optionally contain a light beam forming optical system, specific for a given spectrum analyzing device, spectrum specific dispersing or light filtering element, a light beam forming system for dispersed light and a wavelength specific array of the photodetectors.

The signal from each array is read by one or more specialized electronics boards (29), usually specific for each kind of array or detector, and in addition to collection of the signal, performs control of the array by providing proper electrical signals. By means of electrical cables 210 boards are connected to a computer 211 which "supervises" the action of the boards, takes information from the boards, stores it and processes using one of many available chemometric methods (for example PLS or PCR) to convert information collected from arrays into information concerning the chemical composition of the tested sample

- 20 -

and to present it to user in required form (graphs or any other signal). It is important to appreciate that number n_1 and kind of light sources is selected to provide illumination in all spectral bands of the interest in both AV and IR ranges, and in general can be different from number n_2 of the spectrum analyzing devices (spectrometers, for example) selected to secure detection in these spectral bands with required resolution.

While the present invention has been described with reference to what are presently considered to be preferred examples, it is to be understood that the invention is not limited to the disclosed examples. To the contrary, the invention is intended to cover various modifications and equivalents included within the spirit and scope of the appended claims.

All publications, patents and patent applications referred to herein are incorporated by reference in their entirety to the same extent as if each individual publication, patent or patent application was specifically and individually indicated to be incorporated by reference in its entirety.

- 21 -

WE CLAIM:

1. A method for determining a concentration of a constituent in a sample comprising the steps of:

5 irradiating the sample with a broad spectrum of radiation from the adjacent visible and near infrared (AV/NIR) region;

collecting radiation after the radiation has been directed onto the sample;

10 dispersing the collected radiation into a dispersed spectrum of component wavelengths onto a detector of the AV/NIR, the detector of the AV/NIR taking measurements of at least one of transmitted or reflected radiation from the collected radiation; and transferring the measurements to a processor;

15 irradiating the sample with a broad spectrum of radiation in the longer wavelength near infrared (LWNIR) region; detecting one or more bands of radiation after the radiation has been directed onto the sample with a detector of the LWNIR, the detector of the LWNIR taking measurements of at least one of transmitted or reflected radiation ; and

20 transferring the measurements to a processor;
based on the measurements and one or more calibration algorithms, the processor calculating the concentration of said constituent in said sample.

25 2. A method according to claim 1 wherein one or more separate energy sources are used to provide radiation.

30 3. A method according to either claim 1 or 2 wherein the detector of the AV/NIR is one or more spectral instruments with an array of silicon detectors and the detector of LWNIR is one or more spectral instruments with a separate array of infrared sensitive detectors for each band of radiation.

35 4. A method according to either claim 1 or 2 wherein the detector of the AV/NIR is one or more spectral instruments with an array of silicon detectors and the detector of LWNIR is one or more spectral

- 22 -

instruments with an array of infrared sensitive detectors and measurements for each band of radiation are taken from appropriate members of the array of infrared sensitive detectors.

5 5. A method according to any one of claims 1-4 wherein the infrared sensitive detectors are InGaAs detectors.

10 6. A method according to any of claims 1-5 wherein the spectrometers with silicon detectors arrays register light in the all of the visible, visible/infrared and adjacent to visible infrared ranges within the spectral sensitivity range of the detectors.

15 7. A method according to any of claims 1-6 wherein the spectrometers with infrared sensitive detectors register light in the separate infrared ranges within their spectral sensitivity range.

20 8. A method according to any of claims 1-7 wherein all detectors register light in their respectable sensitivity ranges virtually simultaneously.

9. A method for determining a concentration of a constituent in a sample comprising the steps of:

25 irradiating the sample with a broad spectrum of radiation from the AV/NIR region;

collecting radiation after the radiation has been directed onto the sample;

30 dispersing the collected radiation into a dispersed spectrum of component wavelengths onto a detector of the AV/NIR, the detector of the AV/NIR taking measurements of at least one of transmitted and reflected radiation from the collected radiation; and transferring the measurements to a processor;

35 irradiating the sample with one or more bands of radiation in the LWNIR region; detecting the one or more bands of radiation after the radiation has been directed onto the sample with a detector of the LWNIR, the detector of the LWNIR taking measurements of at least one of transmitted and reflected radiation ; and

- 23 -

transferring the measurements to a processor;
based on the measurements and one or more calibration algorithms,
the processor calculating the concentration of said constituent in said
sample.

5

10. A method according to claim 9 wherein one or more separate
energy sources are used to provide radiation of required spectral
content.

10

11. A method according to either claim 9 or 10 wherein the detector
of the AV/NIR is one or more spectral instruments with an array of
silicon detectors and the detector of LWNIR is one or more spectral
instruments with a separate array of infrared sensitive detectors for
each band of radiation.

15

12. A method according to either claim 9 or 10 wherein the detector
of the AV/NIR is one or more spectral instruments with an array of
silicon detectors and the detector of LWNIR is one or more spectral
instruments with an array of infrared sensitive detectors and
measurements for each band of radiation are taken from appropriate
members of the array of infrared sensitive detectors.

20

13. A method according to any one of claims 9-12 wherein the
infrared sensitive detectors are InGaAs detectors.

25

14. A method according to any of claims 9-13 wherein the
spectrometers with silicon detectors arrays register light in the all of
the visible, visible/infrared and adjacent to visible infrared ranges
within the spectral sensitivity range of the detectors.

30

15. A method according to any of claims 9-14 wherein the
spectrometers with infrared sensitive detectors register light in the
separate infrared ranges within their spectral sensitivity range.

- 24 -

16. A method according to any of claims 9-15 wherein all detectors register light in their respectable sensitivity ranges virtually simultaneously.

17. A method for determining a concentration of a constituent in a sample comprising the steps of:

irradiating the sample with a broad spectrum of radiation from the AV/NIR region;

collecting radiation after the radiation has been directed onto the sample;

dispersing the collected radiation into a dispersed spectrum of component wavelengths onto a detector of the AV/NIR, the detector of the AV/NIR taking measurements of at least one of transmitted and reflected radiation from the collected radiation; and transferring the measurements to a processor;

irradiating the sample with a broad spectrum of radiation from the LWNIR region; collecting radiation after the radiation has been directed onto the sample;

dispersing the collected radiation into a dispersed spectrum of bands of radiation onto a detector of the LWNIR, the detector of the LWNIR taking measurements of at least one of transmitted and reflected radiation; and

transferring the measurements to a processor; based on the measurements and one or more calibration algorithms, the processor calculating the concentration of said constituent in said sample.

18. A method according to claim 17 wherein one or more separate energy sources are used to provide radiation of required spectral content.

19. A method according to either claim 17 or 18 wherein the detector of the AV/NIR is one or more spectral instruments with an array of silicon detectors and the detector of LWNIR is one or more spectral instruments with a separate array of infrared sensitive detectors for each band of radiation.

- - 25 -

20. A method according to either claim 17 or 18 wherein the detector of the AV/NIR is one or more spectral instruments with an array of silicon detectors and the detector of LWNIR is one or more spectral instruments with an array of infrared sensitive detectors and measurements for each band of radiation are taken from appropriate members of the array of infrared sensitive detectors.

21. A method according to any one of claims 17-20 wherein the infrared sensitive detectors are InGaAs detectors.

22. A method according to any of claims 17-21 wherein the spectrometers with silicon detectors arrays register light in the all of the visible, visible/infrared and adjacent to visible infrared ranges within the spectral sensitivity range of the detectors.

23. A method according to any of claims 17-22 wherein the spectrometers with infrared sensitive detectors register light in the separate infrared ranges within their spectral sensitivity range.

24. A method according to any of claims 17-23 wherein all detectors register light in their respectable sensitivity ranges virtually simultaneously.

25. A method according to any one of claims 1-24 wherein the sample is a finger of a subject.

1/2

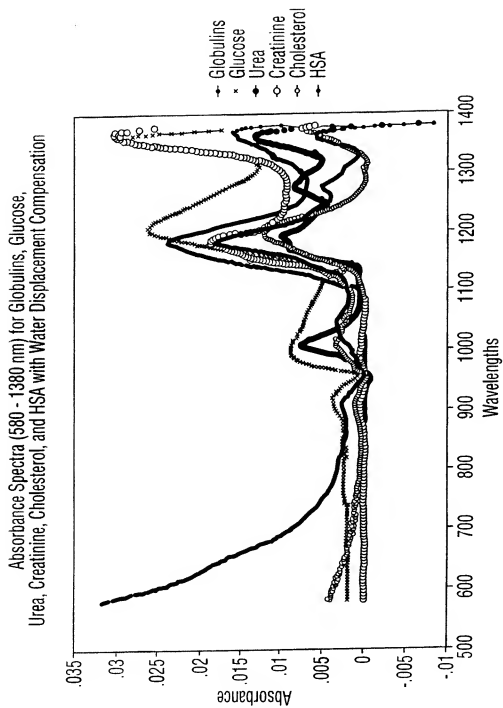
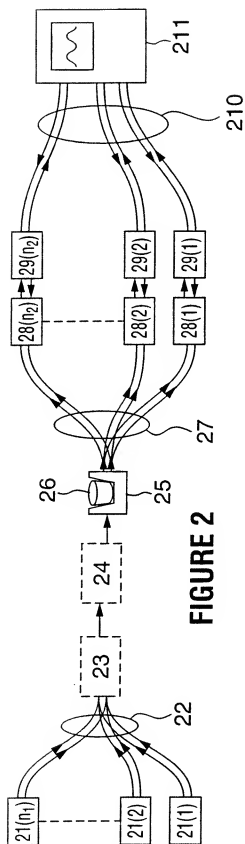


FIGURE 1

SUBSTITUTE SHEET (RULE 26)

2/2

**FIGURE 2**

INTERNATIONAL SEARCH REPORT

International Application No.

PCT/CA 00/01003

A. CLASSIFICATION OF SUBJECT MATTER

IPC 7 G01N21/35 G01N21/31 A61B5/00

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 G01N A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and where practical, search terms used)

EPO-Internal, WPI Data

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	WO 96 37259 A (DOMJAN GYULA ;GOEDOELLE LASZLO (HU); GYARMATI LASZLO (HU); JAKO JA) 28 November 1996 (1996-11-28) page 7, line 4-15 page 9, line 21 -page 11, line 5 page 15, line 10-30; figures 1-3 ---	1-25
X	US 5 747 806 A (KHALIL GAMAL ET AL) 5 May 1998 (1998-05-05) column 3, line 32-53 column 6, line 62-66 column 9, line 16 -column 10, line 46 column 11, line 14-23 column 12, line 59-61; figures 1-3 --- -/-	1,2, 8-10, 16-18,24

☒ Further documents are listed in the continuation of box C

☒ Patent family members are listed in annex

* Special categories of cited documents

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claims or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance, the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance, the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"S" document member of the same patent family

Date of the actual completion of the international search

22 December 2000

Date of making of the international search report

05/01/2001

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel: (+31-70) 340-2040, Tx: 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Meyer, F

INTERNATIONAL SEARCH REPORT

Inter nal Application No

PCT/CA 00/01003

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category	Citation of document with indication where appropriate of the relevant passages	Relevant to claim No
A	US 5 743 262 A (LEPPER JR JAMES M ET AL) 28 April 1998 (1998-04-28) column 3, line 29-55 column 5, line 46 -column 8, line 5 column 13, line 34-41: figures 5,11 ----	1,9,17
A	US 5 818 048 A (GUTHERMANN HOWARD E ET AL) 6 October 1998 (1998-10-06) column 7, line 38-56 column 11, line 10 -column 14, line 36: figures 2,4,5 ----	1,9,17
A	US 5 361 758 A (HALL JEFFREY W ET AL) 8 November 1994 (1994-11-08) cited in the application the whole document -----	1,9,17

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/CA 00/01003

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 9637259 A	28-11-1996	HU 216847 B AU 5842596 A EP 0828533 A US 5974337 A	28-12-1999 11-12-1996 18-03-1998 26-10-1999
US 5747806 A	05-05-1998	AU 713502 B AU 1844997 A CA 2244111 A CN 1214769 A CZ 9802392 A EP 0877926 A JP 11506207 T NZ 331158 A PL 328060 A US 5945676 A WO 9728438 A	02-12-1999 22-08-1997 07-08-1997 21-04-1999 14-07-1999 18-11-1998 02-06-1999 28-10-1999 04-01-1999 31-08-1999 07-08-1997
US 5743262 A	28-04-1998	AU 715345 B AU 6033296 A CA 2221384 A CN 1192273 A EP 0830582 A JP 11505451 T US 6110522 A WO 9641151 A	20-01-2000 30-12-1996 19-12-1996 02-09-1998 25-03-1998 21-05-1999 29-08-2000 19-12-1996
US 5818048 A	06-10-1998	US 5434412 A US 5424545 A US 5321265 A WO 9614567 A US 6028311 A US 5672875 A US 6064065 A AU 689137 B AU 7842894 A CA 2173200 A DE 69423503 D DE 69423503 T EP 0721579 A EP 0967477 A ES 2145843 T JP 9503585 T WO 9510038 A US 5818044 A CA 2180128 A EP 0742897 A JP 9510884 T WO 9519562 A AU 4670293 A CA 2140239 A DE 69328363 D DE 69328363 T EP 0650591 A EP 0967478 A ES 2146232 T JP 8502350 T WO 9402837 A	18-07-1995 13-06-1995 14-06-1994 17-05-1996 22-02-2000 30-09-1997 16-05-2000 26-03-1998 01-05-1995 13-04-1995 20-04-2000 29-06-2000 17-07-1996 29-12-1999 16-07-2000 08-04-1997 13-04-1995 06-10-1998 20-07-1995 20-11-1996 04-11-1997 20-07-1995 14-02-1994 03-02-1994 18-05-2000 10-08-2000 03-05-1995 29-12-1999 01-08-2000 12-03-1996 03-02-1994

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/CA 00/01003

Patent document
cited in search report

Publication
date

Patent family
member(s)

Publication
date

US 5361758

A

08-11-1994

NONE